



Volume 7 Issue 8,
September 2021

Copyright

©2021 Zubaer AHMED et al. This is an open access article distributed under the terms of the Creative Commons Attribution License, which permits unrestricted use, distribution, and reproduction in any medium, provided the original author and source are credited



Citation

Zubaer AHMED et al. (2021), Effect of Conditioning and 3-Year Aging on the Bond Strength and Interfacial Morphology of Glass-Ionomer Cement Bonded to Dentin Int J Dent & Ora Hea. 7:8, 86-93

ISSN 2471-657X

Published by
Biocore Group |
<https://www.biocoreopen.org/ijidoh/archive.php>

International Journal of Dentistry and Oral Health

Research Article

Effect of Conditioning and 3-Year Aging on the Bond Strength and Interfacial Morphology of Glass-Ionomer Cement Bonded to Dentin

Zubaer AHMED^{1,2}, Shamme Akter RIME², Hidehiko SAN⁰, Shuhei HOSHIKA^{2*}

¹ Department of Conservative Dentistry and Endodontics, Mandy Dental College and Hospital, Dhaka, Bangladesh.

² Department of Restorative Dentistry, Division of Oral Health Science, Hokkaido University, Graduate School of Dental Medicine, Kita 13, Nishi 7, Kita-ku, Sapporo 060-8586, Japan.

Corresponding author: Shuhei HOSHIKA

Department of Restorative Dentistry, Graduate School of Dental Medicine, Hokkaido University, Kita 13, Nishi 7, Kita-ku, Sapporo 060-8586, Japan E-mail: hoshika@den.hokudai.ac.jp

Article History: Received: August 06, 2021;
Accepted: September 01, 2021;
Published: September 28, 2021.

Abstract

Objectives: The purpose of this study was to determine the bond stability and the change in interfacial ultra-structure of a conventional glass-ionomer cement bonded to dentin, with and without pre-treatment using a polyalkenoic acid conditioner.

Material and Methods: The occlusal dentin surfaces of six teeth were ground flat. Glass-ionomer cement was bonded to the surfaces either with or without polyalkenoic acid conditioning. The teeth were sectioned into 1-mm² stick-shaped specimens. The specimens obtained were randomly assigned to two groups with different periods of storage in water: 1-week and 3-year. The micro-tensile bond strength (μ TBS) was determined for each storage time. Additional specimens were prepared for interfacial analysis by using Scanning Electron Microscopy (SEM); they were produced with or without prior polyalkenoic acid conditioning in the same way as in the μ TBS test.

Results: There was no significant difference in μ TBS to conditioned dentin and non-conditioned dentin ($p > 0.05$). The failures appeared to be of a mixed nature, although aging caused more areas of cohesive than adhesive failure in both groups.

Conclusions: Aging did not reduce the bond strength of the conventional glass-ionomer cement to dentin with or without the use of a polyalkenoic acid conditioner. Remineralized dentin layer were observed in both conditioned and unconditioned 3-years specimens.

Keywords

Adhesion, Dentin, Glass-ionomer cement, Micro-tensile bond strength, Scanning Electron Microscopy.

Declaration of Conflicting Interest

This research did not receive any specific grant from funding agencies in the public, commercial, or not-for-profit sectors.

Acknowledgment

The authors acknowledge the technical supports provided by the department of Restorative dentistry, Hokkaido University and Ms. Ushijima N for this study and would like to thanks her.

Introduction

Now a days we can carry out the tooth adhesion to enamel and dentin to an advance level by means of dental restorative materials such as glass-ionomer cement (GIC) and resin-based composites. GIC are bioactive and independent. Bio- compatibility or bioactivity, which is now a big trend in restorative dentistry. [1] When they actively stimulate or direct tissue responses and they can control interactions with microbiological species besides their primary function of restoring or replacing missing tooth structure then dental restorative materials should be called "bioactive" materials. [2] Remineralization and anti-microbial properties are the two major aspects of bioactivity. Those materials which are bioactive containing calcium silicate, [3] [4] calcium phosphate, [5] hydroxyapatite [6] [7] etc, were reported to have remineralization ability. Regarding the anti-microbial property, the release of compounds with antibiotic-like efficacy were used to inhibit oral bacteria and biofilm. [8] [9]

GIC is one of a dental bioactive material. [10] [11] It has a pH-buffering capacity, as it releases fluoride proportionally to the acidity. [12] [13] It has also both remineralization and anti-microbial ability [14] [15] [16] [17] and it has been commonly used in the Atraumatic Restorative Treatment (ART) technique in developing countries for a long time. [18] GIC can bond chemically to hydroxyapatite (HAp) and does not require light curing. Although it has a less demanding technique than resin-based restorations like resin composite, but often used clinically because of operator friendly technique, cost effectiveness and adhere directly to dental hard tissues even in a moist environment. It has a major advantage over resin composite that it has no conversion shrinkage and still an effective material in the case of deep cavities. [19] [20]

GICs achieve such clinically suitable results and lowest annual failure rate in vivo even the bond strength of GIC may be much weaker compared with resin-based materials. [21] Some studies have reported certain GICs adhere to tooth structure without pre-treatment [22] [23] but some other studies have reported by using surface pre-treatment the adhesion of GICs over dentin is improving. [24] [25]

The purpose of this study was to assess the adhesion of the GIC-dentin by means of bond strength and interfacial morphology after 1-week and 3-year of aging, with and without surface pre-treatment. The null hypothesis tested in this study was that pre-treatment of dentin using a polyalkenoic acid conditioner did not affect the long-term durability of a conventional GIC.

Materials and methods

1. Microtensile bond strength test (μ TBS)

The bond strength to dentin was determined using a standard micro-tensile bond strength test. [26] The materials used in this study are shown in Table 1. Six human molars, stored in a 0.5% chloramine T solution, were used within 1 month of extraction. The protocol of this research was approved by the Commission for Medical Ethics of Hokkaido University. The extracted molars were sectioned at the mid-coronal portion to create a flat dentin surface by using a low-speed diamond saw (Isomet 1000, Buehler, Lake Bluff, IL, USA). A standard smear layer was produced using #600 grit silicon carbide paper. The teeth were randomly divided into two groups of three teeth each. Prior to the application of the GIC, the dentin surface of the specimens in one group was pre-treated with a polyalkenoic acid conditioner (Cavity Conditioner, GC, Tokyo, Japan). This contains 3% Aluminum chloride as well as 20% polyalkenoic acid. The specimens in the other group did not receive any pre-treatment. The dentin surface was subsequently built up free-hand and in bulk with a conventional GIC (Fuji IX GP Extra, GC, Tokyo, Japan) to a height of 5–6 mm.

Product name	Composition
Cavity conditioner (GC, Tokyo, Japan)	20% Polyacrylic acid, Distilled water, Aluminum chloride hydrate, Food additive Blue No. 1
Fuji IX GP Extra (GC)	Polyacrylic acid, Aluminosilicate glass, Proprietary ingredient

Table: The materials used in this study

After 1-week of storage in distilled water at 37°C, the specimens were sectioned perpendicular to the bonding surface, to obtain 1-mm² stick-shaped micro-specimens using an Isomet saw. The specimens were then randomly assigned to four groups (10 specimens each) according to age/storage time: 1-week and 3-year, i.e. the 1-week specimens were tested after sectioning while the rest continued in storage to 3-year. An absolute 3 teeth per experimental group with appropriate consideration of tooth dependency are required if the specimen is used as the statistical unit.^[27] At the relevant time period, the micro-specimens were fixed to a jig with cyanoacrylate glue (Model Repair II Blue, Dentsply-Sankin, Ohtawara, Japan) and stressed in a testing device (EZ-test, Shimadzu, Kyoto, Japan) at a crosshead speed of 1 mm/min until failure occurred. The μ TBS was calculated in MPa, derived by dividing the force applied (in N) at the time of fracture by the bonded area (in mm²). Statistical analysis was performed using one-way ANOVA ($\alpha = 0.05$) and post hoc Tukey-Kramer multiple comparisons tests. The mode of failure was determined by examining the fractured surface at a magnification of $\times 80$ using a stereo-microscope (Wild M5A, Heerbrugg, Switzerland).

2. Scanning electron microscopy (SEM) Interface analysis

Additional GIC specimens were prepared for examination using SEM (S-4000, HITACHI, Tokyo, Japan). For this, a further four teeth were randomly divided into two groups of two teeth each; the dentin was pre-treated with polyalkenoic acid conditioner in one group but not in the other. The procedure of bonding the GIC to dentin was the same as previously described in the μ TBS test, before storage in distilled water for 1-week and 3-year at 37 °C. The GIC-bonded dentin specimens were sectioned perpendicular to the GIC/dentin interface using an Isomet diamond saw. From each tooth, seven or eight rectangular sections, of approximately 1 mm thickness each, were obtained. After storage for each time period, SEM sample preparation was performed in accordance with common procedures following a protocol described by Saikaew et al. [28] Specimen were dried for 24h. They were then fixed on aluminum stubs and coated with Pt-Pd alloy (E-1030, HITACHI, Tokyo, Japan) for 150 s. The GIC/dentin interface in each section was observed by SEM (S-4000, HITACHI) at an accelerating voltage of 10 kV. First, all the surfaces were examined at lower magnification ($\times 80$). Special features were further observed at $\times 800$ and $\times 2,000$ magnifications.

Results

1. Microtensile bond strength (μ TBS)

The mean μ TBSs are presented in Figure 1. No pre-testing failures (ptfs) were found in this study. There was no significant difference in μ TBS when Cavity Conditioner was used at each time period ($p > 0.05$). In addition, 3-year water storage did not show significant difference between conditioned and non-conditioned dentin in terms of μ TBS results.

2. SEM failure analysis

At 1-week, the failure patterns were generally of a 'mixed' nature, involving areas that failed at the interface and areas that failed cohesively within the GIC, for both the conditioned and non-conditioned groups. At 3-year, while the failure was still of a mixed nature, there was a tendency for more areas of cohesive failure. It appeared that aging of both conditioned and non-conditioned specimens caused them to fail slightly more frequently cohesively within the GIC.

3. SEM interface analysis

Representative SEM images of the GIC/dentin interface with polyalkenoic acid conditioning stored for 1-week and 3-year are shown in Figure 2(a-d), while GIC/dentin with non-conditioned interface for 1-week and 3-year are shown in Figure 3(a-d).

With polyalkenoic acid conditioning, a shallow demineralized dentin layer was seen at the dentin-conditioned interface in 1-week (Figure 2a & 2c). However, remineralized dentin layer was seen on 3-year image (Figure 2b & 2d). Additionally, on GIC surface area, glass-ionomer tags were seen on 1-week specimen's image (Figure 2a & 2c) whereas glass-ionomer tags were not visible on 3-year specimen's image (Figure 2b & 2d). On 1-week, dentinal tubules were visible (Fig. 2a, 2c) while on 3-year there were no dentinal tubules seen (Figure 2b, 2d). The GIC surface area were drier and several cracks were visible in long term stored samples (Figure 2b, 2d). The conditioned interface has high viscous, so that the layer of interface is prominent. After interface observing, there were no sign of interface degradation in 3-year samples.

Representative SEM images of the GIC/dentin interface without polyalkenoic acid conditioning stored for 1-week and 3-year are shown in Figure 3(a-d). The GIC was closely attached to the dentin surface without any intervening layers detected. However, remineralized dentin layer might be seen on 3-year image Figure 3 (b,d). No dentinal tubules were seen on both 1-week and 3-year samples. It is difficult to distinguish intact-like dentin and remineralized dentin on 3-year samples. The bond appeared intact. No clear signs of bond degradation were observed after 3-year of water storage.

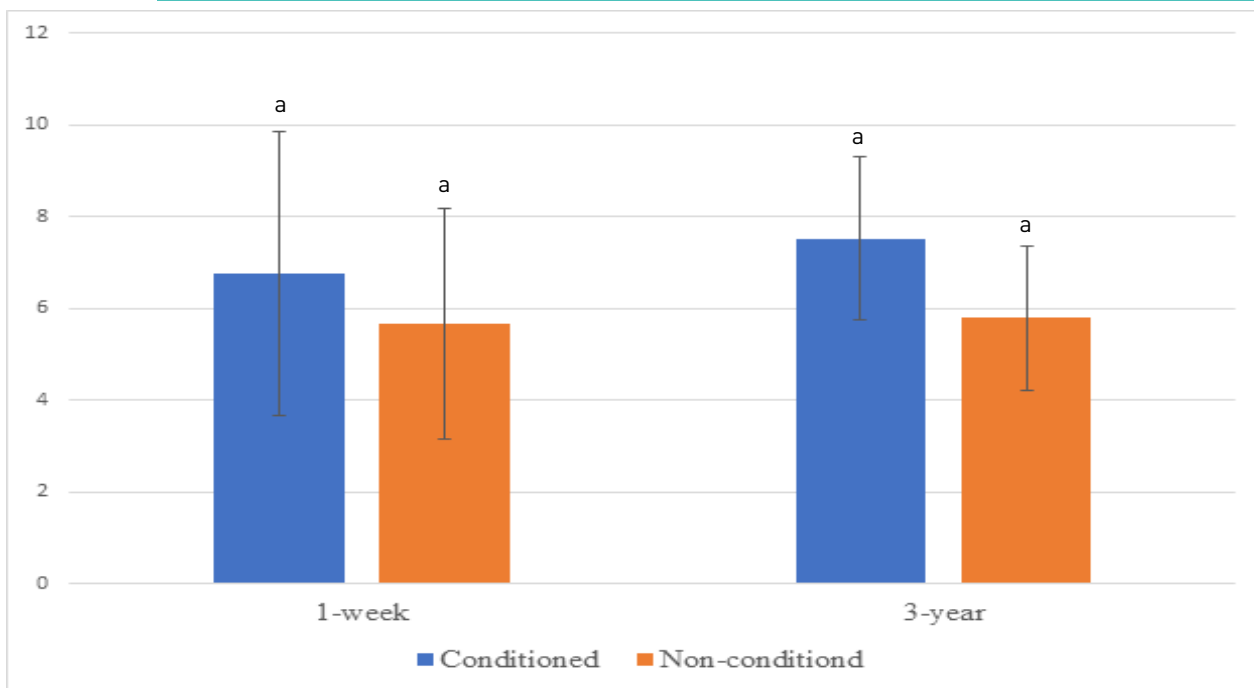


Figure 1: Micro-tensile bond strength of GIC bonded to polyalkenoic acid conditioned (Cavity Conditioner) and non-conditioned dentin for 1 week and 3 year. Mean µTBS are presented in MPa. n = 10. The same letters indicate no statistically significant difference ($p > 0.05$).

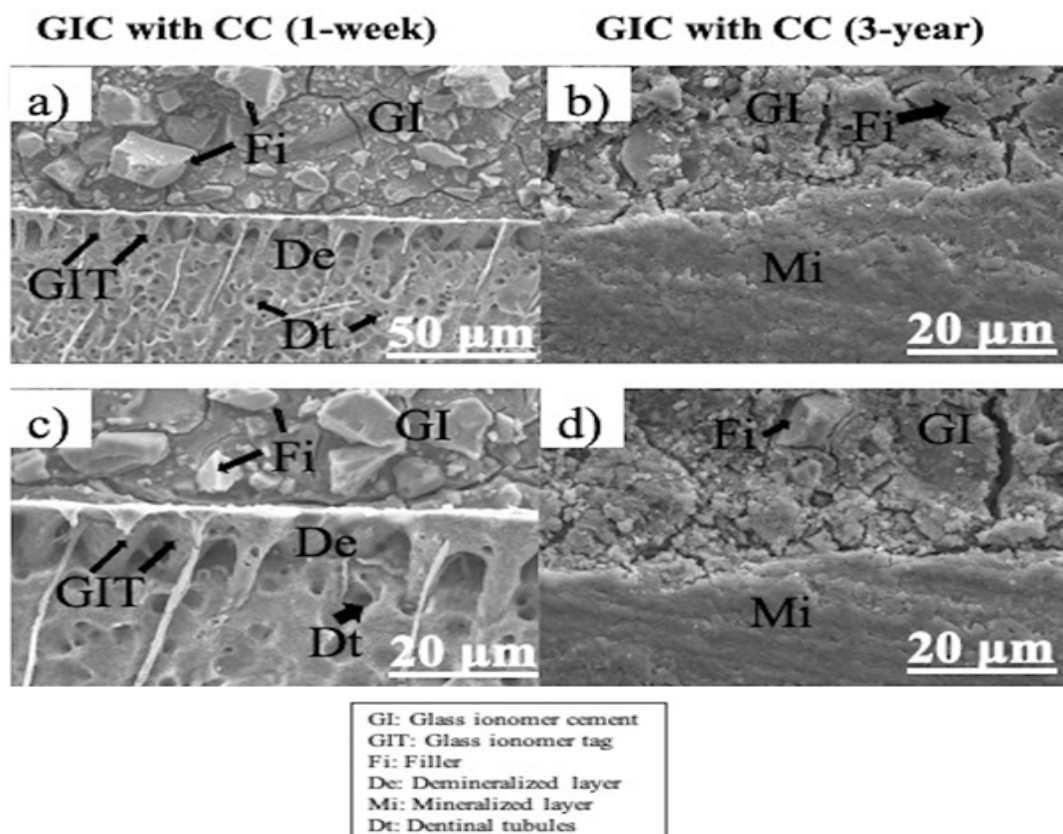


Figure 2: Representative SEM photomicrographs of the GIC/dentin interface with polyalkenoic acid conditioning using Cavity Conditioner stored for 1-week and 3-year (a,b,c,d). a = x800 and b, c, d = x2000. A partially demineralized dentin layer was formed on 1-week stored samples (Fig. 2a, 2c) whereas remineralized dentin layer was formed on 3-year samples (Fig. 2b, 2d). On 1-week, dental tubules were visible (Fig. 2a, 2c) while on 3-year there were no dental tubules seen (Fig. 2b, 2d). The GIC surface area were drier and several cracks were visible in long term stored samples (Fig. 2b, 2d). [GI = Glass ionomer cement; GIT = Glass ionomer tag; Fi = Filler; De = Demineralized Layer; Mi = Mineralized layer; Dt = Dental tubules].

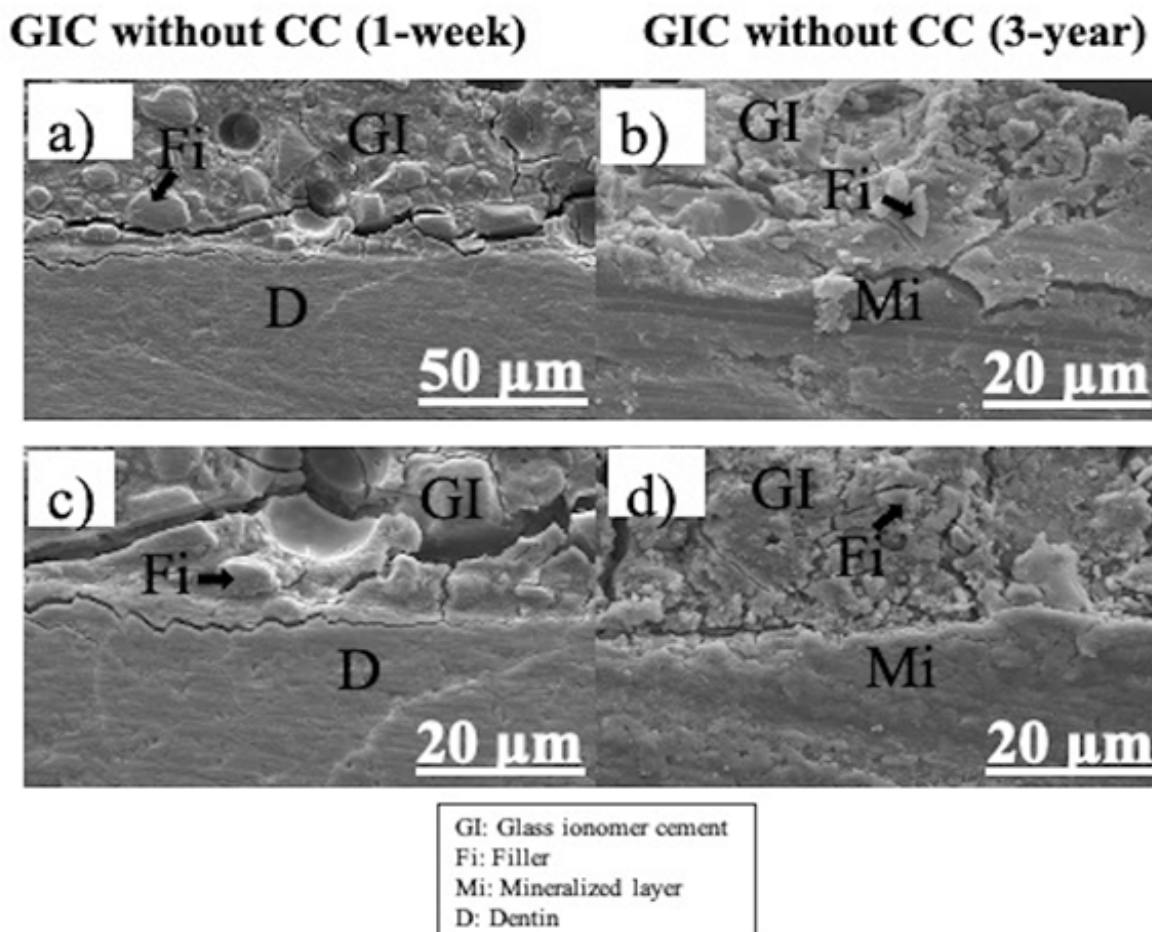


Figure 3: Representative SEM photomicrographs of the GIC/dentin interface without polyalkenoic acid conditioning stored for 1-week and 3-year (a, b, c, d). a, b, d = x2000 and c = x800. Observed intact-like dentin on 1-week and Mineralized dentin layer was observed on 3-year, but no dentinal tubules were seen on both 1-week and 3-year samples. Therefore, it is difficult to distinguish intact-like dentin and remineralized dentin on 3-year samples. However, on GIC surface area, several fillers were observed on both 1-week and 3-year storage time. [GI = Glass ionomer cement; Fi = Filler; Mi: Mineralized layer, D: Dentin].

Discussion

The clinical ability of dental materials can be envisaged at laboratory settings by using μ TBS test, especially after subjecting the specimens to aging challenges.^{[29] [30]} In this study, by using μ TBS test and SEM, the interfacial ultrastructure of GIC/dentin bonds and the long-term durability was studied respectively. From the μ TBS test, there was no significantly difference between immediate and after 3 years of aging and the use of cavity conditioner did not make a significant difference to the μ TBS ($p > 0.05$). As cohesive failure within the GIC tends to occur over time, this may be the reason why there was no significant difference in μ TBS. The circumstances is that there was no significant difference in μ TBS even when polyalkenoic acid conditioning was used. Although polyalkenoic acid is still recommended to maximize the ionic reaction with GIC, and to form insoluble calcium salts which facilitates wetting of the surface and increases the contact area.^{[31] [32] [33] [34]}

In recent years, compared to resin-based adhesive interfaces, the interaction of GIC with dentin has been less commonly verified by high-resolution microscopy.^[33] SEM analysis in this study revealed that the interaction of GIC with dentin following some distinct patterns. After bonded with dentin by using polyalkenoic acid, a partially demineralized dentin layer was formed on 1-week stored samples (Fig. 2a, 2c) whereas remineralized dentin layer was formed on 3-year samples (Figure 2b, 2d). On 1-week, dentinal tubules were visible (Figure 2a, 2c) while on 3-year there were no dentinal tubules seen because of the remineralization effect (Figure 2b, 2d). The GIC surface area were dried and several cracks were visible in long term stored samples (Figure 2b, 2d) presumably because GIC has fragile characteristics. The conditioned interface has high viscous, so that the layers of interface is prominent. If we compare with 1-week and 3-year samples, the interface layer of 1-week was more prominent and visible than 3-year. This fact may be attributed due to the maturing effect of GIC, especially as when using polyalkenoic acid conditioning, the reaction of calcium and phosphate ions with GIC was stimulated and the remineralizing

effect may have been supported as well with age. After interface observing, there were no sign of interface degradation in both 1-week and 3-year samples which was same by the previously reported researchers.^{[35] [36]}

When the GIC was applied without polyalkenoic acid conditioning, dentin demineralization was not observed (Figure 3a-3d), Just observed intact-like dentin on 1-week and presumably mineralized dentin layer on 3-year. No dentinal tubules were seen on both 1-week and 3-year samples. Whether with or without cavity conditioner, remineralized layer was seen after 3-year which is remarkable. In addition, according to previous study chemical bonding may occur.^[37] This was also demonstrated from the μ TBS results, when GIC applied without prior polyalkenoic acid conditioning did not able to reveal significantly different bond strength in comparison with the conditioned dentin even though the limited micromechanical interlocking at up to 3-year of aging. In Figure 3(a, b) of un-conditioned specimens, the dentin zone and GIC zone can see without any prime different types of layer and in μ TBS, there were no significant difference between with and without the polyalkenoic acid conditioned group. An ultra-thin demineralized layer at the interface might exist.^[38]

By using conditioners many researchers have shown an increase in the bond strength of GIC to dentin and a decrease in the amount of microleakage.^{[23] [39] [40] [41]} This could be due to the removal of smear layer, elimination of debris, partial demineralization and formation of microprositities in the enamel and dentinal surfaces, enamel rod exposure, which results in an increased surface for microchemical and chemical bonding.^{[39] [40]} Some researchers believe that there is no benefit in applying conditioners because the acidic nature of glass ionomer causes partial dissolution of the smear layer. The conflicting results reported in different studies can be the cause of residual dentin's thickness.^{[22] [23] [42]} GIC was applied with polyalkenoic acid conditioning might be clinically recommended for caries affected dentin, treated with deep dentin and old-aged patient.

Some studies have shown that GIC stored in saliva enhanced surface characteristics comparison with GIC stored in distilled water.^{[43] [44] [45] [46]} From saliva GIC may absorb some inorganic ions and this may improve the surface hardness over time. Further investigations should be conducted to assess the effect of GIC-dentin bond aging within saliva.

From the results of the μ TBS test, pre-treatment of dentin using a polyalkenoic acid conditioner did not affect the long-term durability of a conventional GIC; hence, the null hypothesis should be accepted.

Further research will be conducted to access the effect of GIC-dentin bond aging within saliva and to access the effect of GIC on caries-affected dentin using polyalkenoic acid.

Conclusion

Within the limitations of this in vitro study, Aging did not reduce the bond strength of the conventional GIC to dentin whether the surface was pre-treated with a polyalkenoic acid conditioner or not. Remineralized dentin layer was observed in both conditioned and un-conditioned on 3-year specimens.

References

- [1] Bachoo IK, Seymour D, Brunton P. (2013). A biocompatible and bioactive replacement for dentine: is this a reality? The properties and uses of a novel calcium-based cement. *Br Dent J*, 214(2), E5. [doi: 10.1038/sj.bdj.2013.57. PMID: 23348482].
- [2] Imazato S. (2009). Bio-active restorative materials with antibacterial effects: new dimension of innovation in restorative dentistry. *Dent Mater J*, 28, 11–9. [doi: 10.4012/dmj.28.11. PMID: 19280964].
- [3] Han L, Okiji T. (2013). Bioactivity evaluation of three calcium silicate-based endodontic materials. *Int Endod J*, 46, 808–14. [doi: 10.1111/iej.12062. Epub 2013 Feb 12. PMID: 23402321].
- [4] Niu LN, Jiao K, Wang TD, Zhang W, Camilleri J, Bergeron BE, et al. (2014). A review of the bioactivity of hydraulic calcium silicate cements. *J Dent*, 42, 517–33. [doi: 10.1016/j.jdent.2013.12.015. Epub 2014 Jan 15. PMID: 24440449; PMCID: PMC3995854].
- [5] Zhao J, Liu Y, Sun WB, Zhang H. (2011). Amorphous calcium phosphate and its application in dentistry. *Chem Cent J*, 5, 40. [doi: 10.1186/1752-153X-5-40. PMID: 21740535; PMCID: PMC3143077].
- [6] Tschoppe P, Zandim DL, Martus P, Kielbassa AM. (2011). Enamel and dentine remineralization by nano-hydroxyapatite toothpastes. *J Dent*, 39, 430–7. [doi: 10.1016/j.jdent.2011.03.008. Epub 2011 Apr 8. PMID: 21504777].
- [7] Venkatesan J, Kim SK. (2014). Nano-hydroxyapatite composite biomaterials for bone tissue engineering—a review. *J Biomed Nanotechnol*; 10, 3124–40. [doi: 10.1166/jbn.2014.1893. PMID: 25992432].
- [8] Imazato S, Ma S, Chen JH, Xu HH. (2014). Therapeutic polymers for dental adhesives: loading resins with bio-active components. *Dent Mater*, 30, 97–104. [doi: 10.1016/j.dental.2013.06.003. Epub 2013 Jul 27. PMID: 23899387; PMCID: PMC4312699].
- [9] AydinSevinc , B, Hanley L. (2010). Antibacterial activity of dental composites containing zinc oxide nanoparticles. *J Biomed Mater Res B Appl Biomater*, 94, 22–31. [doi: 10.1002/jbm.b.31620. PMID: 20225252; PMCID: PMC2881188].
- [10] Nicholson JW, Czarnecka B. (2009). Role of aluminum in glass-ionomer dental cements and its biological effects. *J Biomater Appl*, 24, 293-308. [doi: 10.1177/0885328209344441. Epub 2009 Sep 8. PMID: 19737809].

- [11] Sidhu SK, Schmalz G. (2001). The biocompatibility of glass-ionomer cement materials. A status report for the American Journal of Dentistry. *Am J Dent*, 14, 387-396.
- [12] Davidson CL. (2006). Advances in glass-ionomer cements. *J Appl Oral Sci*, 14, 3-9. [doi: 10.1590/s1678-77572006000700002. PMID: 19089079].
- [13] Ngo HC, Mount G, Mc Intyre J, Tuisuva J, Von Doussa RJ. (2006). Chemical exchange between glass-ionomer restorations and residual carious dentine in permanent molars: an in vivo study. *J Dent*, 34, 608-613. [doi: 10.1016/j.jdent.2005.12.012. Epub 2006 Mar 15. PMID: 16540227].
- [14] da Silva RC, Zuanon AC, Spolidorio DM, Campos JA. (2007). Antibacterial activity of four glass ionomer cements used in atraumatic restorative treatment. *J Mater Sci Mater Med*, 18, 1859-62. [doi: 10.1007/s10856-007-3035-4. Epub 2007 May 12. PMID: 17497079].
- [15] Luczaj-Cepowicz E, Marczuk-Kolada G, Zalewska A, Pawin ska M, Leszczyn ska K. (2014). Antibacterial activity of selected glass ionomer cements. *Postepy Hig Med Dosw (Online)*, 68, 23-8. [doi: 10.5604/17322693.1086069. PMID: 24491892].
- [16] Naik RG, Dodamani AS, Khairnar MR, Jadhav HC, Deshmukh MA. (2016). Comparative assessment of antibacterial activity of different glass ionomer cements on cariogenic bacteria. *Restor Dent Endod*, 41, 278-82. [doi: 10.5395/rde.2016.41.4.278. Epub 2016 Sep 20. PMID: 27847749; PMCID: PMC5107429].
- [17] Tüzüner T, Dimkov A, Nicholson JW. (2019). The effect of antimicrobial additives on the properties of dental glass-ionomer cements: a review. *Acta Biomater Odontol Scand*, 5, 9-21. [doi: 10.1080/23337931.2018.1539623. PMID: 30652117; PMCID: PMC6327935].
- [18] Frencken JE. (2010). The ART approach using glass-ionomers in relation to global oral health care. *Dent Mater*, 26, 1-6. [doi: 10.1016/j.dental.2009.08.013. PMID: 19804903].
- [19] Francois P, Vennat E, Le Goff S, Ruscassier N, Attal JP, Dursun E. (2019). Shear bond strength and interface analysis between a resin composite and a recent high-viscous glass ionomer cement bonded with various adhesive systems. *Clin Oral Investig*, 23, 2599-608. [doi: 10.1007/s00784-018-2678-5. Epub 2018 Oct 13. PMID: 30317399].
- [20] Paula AM, Boing TF, Wambier LM, Hanzen TA, Loguercio AD, Armas-Vega A, Reis A. (2019). Clinical performance of non-cariou cervical restorations restored with the "Sandwich technique" and composite resin: a systematic review and meta-analysis. *J Adhes Dent*, 21, 497-508. [doi: 10.3290/j.jad.a43696. PMID: 31802065].
- [21] Peumans M, De Munck J, Mine A, Van Meerbeek B. (2014). Clinical effectiveness of contemporary adhesives for the restoration of non-cariou cervical lesions. A systematic review. *Dent Mater*, 30, 1089-103. [doi: 10.1016/j.dental.2014.07.007. Epub 2014 Aug 3. PMID: 25091726].
- [22] Hewlett ER, Caputo AA, Wrobel DC. (1991). Glass ionomer bond strength and treatment of dentin with polyacrylic acid. *J Prosthet Dent*, 66, 767-72. [doi: 10.1016/0022-3913(91)90412-p. PMID: 1805026].
- [23] Tanumiharja M, Burrow MF, Tyas MJ. (2000). Microtensile bond strengths of glass ionomer (polyalkenoate) cements to dentine using four conditioners. *J Dent*, 28, 361-6. [doi: 10.1016/s0300-5712(00)00009-9. PMID: 10785303].
- [24] Cook NB, Feitosa SA, Patel A, Alfawaz Y, Eckert GJ, Bottino MC. (2015). Bonding ability of paste-paste glass ionomer systems to tooth structure: in vitro studies. *Oper Dent*, 40, 304-12. [doi: 10.2341/14-030-L. Epub 2014 Dec 23. Erratum in: *Oper Dent*. 2016 Jan-Feb;41(1):111-3. PMID: 25535780].
- [25] Powis DR, Follerås T, Merson SA, Wilson AD. (1982). Improved adhesion of a glassionomer cement to dentin and enamel. *J Dent Res*, 61, 1416-22.
- [26] Sano H, Shono T, Sonoda H, Takatsu T, Ciucchi B, Carvalho R, et al. (1994). Relationship between surface area for adhesion and tensile bond strength—evaluation of a micro-tensile bond test. *Dent Mater*, 10, 236-40. [doi: 10.1016/0109-5641(94)90067-1. PMID: 7664990].
- [27] Armstrong S, Breschi L, Özcan M, Pfeifferkorn F, Ferrari M, Van Meerbeek B. (2017). Academy of Dental Materials guidance on in vitro testing of dental composite bonding effectiveness to dentin/enamel using micro-tensile bond strength (μ TBS) approach. *Dent Mater*, 33, 133-43. [doi: 10.1016/j.dental.2016.11.015. Epub 2016 Dec 20. PMID: 28007396].
- [28] Saikaew P, Chowdhury AF, Fukuyama M, Kakuda S, Carvalho 292. RM, Sano H. (2016). The effect of dentine surface preparation and reduced application time of adhesive on bonding strength. *J Dent*, 47, 63-70. [doi: 10.1016/j.jdent.2016.02.001. Epub 2016 Feb 5. PMID: 26855030].
- [29] Van Meerbeek B, Peumans M, Poitevin A, Mine A, Van Ende A, Neves A, De Munck J. (2010). Relationship between bond-strength tests and clinical outcomes. *Dent Mater*, 26, e100-e121. [doi: 10.1016/j.dental.2009.11.148. Epub 2009 Dec 16. PMID: 20006379].
- [30] Akter RS, Ahmed Z, Yamauti M, Carvalho RM, Chowdhury AFMA, Sano H. (2021). Effects of remaining dentin thickness, smear layer and aging on the bond strengths of contemporary universal adhesives to dentin. *Dent Mater J*, 40(2), 538-546. [doi: 10.4012/dmj.2019-436. Epub 2020 Dec 17. PMID: 33328395].
- [31] Powis DR, Follerås T, Merson SA, Wilson AD. (1982). Improved adhesion of a glassionomer cement to dentin and enamel. *J Dent Res*, 61, 1416-1422.
- [32] Erickson RL, Glasspoole EA. (1994). Bonding on tooth structure: a comparison of glass-ionomer and composite-resin systems. *J Esth Dent*, 6, 227-44. [doi: 10.1111/j.1708-8240.1994.tb00864.x. PMID: 8593220].
- [33] Hoshika S, De Munck J, Sano H, Sidhu SK, Van Meerbeek B. (2015). Effect of conditioning and aging on the bond strength and interfacial morphology of glass-ionomer cement bonded to dentin. *J Adhes Dent*, 17, 141-6. [doi: 10.3290/j.jad.a33994. PMID: 25859569].

- [34] Pereira LC, Nunes MC, Dibb RG, Powers JM, Roulet JF, Navarro MF. (2002). Mechanical properties and bond strength of glass-ionomer cements. *J Adhes Dent*, 4, 73–80.
- [35] Marleen Peumans, Bart Van Meerbeek, Paul Lambrechts, Guido Vanh. (2003). Two-year clinical effectiveness of a resin-modified glass-ionomer adhesive. *J Dent*, 16(6), 363-8.
- [36] E. Coutinho, M.V. Cardoso, J.De Munck, A.A. Neves, K.L. Van Landuyt, A. Poitevin, M. Peumans, P.Lambrechts, B. Van Meerbeek. (2009). Bonding effectiveness and interfacial characterization of a nano-filled resin-modified glass-ionomer. *Dent Mater*, 25(11), 1347-1357. [doi: 10.1016/j.dental.2009.06.004. PMID: 19595446].
- [37] Coutinho E, Yoshida Y, Inoue S, Fukuda R, Snauwaert J, Nakayama Y, De Munck J, Lambrechts P, Suzuki K, Van Meerbeek B. (2007). Gel phase formation at resin-modified glass-ionomer/tooth interfaces. *J Dent Res*, 86, 656-661. [doi: 10.1177/154405910708600714. PMID: 17586714].
- [38] Shuhei Hoshika, Shihchun Ting, Zubaer Ahmed, Chen Fei, Norihito Sakaguchi, Bart Van Meerbeek, Hidehiko Sano. (2020). Effect of conditioning and 1 year aging on the bond strength and interfacial morphology of glass-ionomer cement bonded to dentin. *Dent Mater*, 37(1), 106-112. [doi: 10.1016/j.dental.2020.10.016. Epub 2020 Nov 21. PMID: 33229039].
- [39] Yilmaz Y, Gurbuz T, Kocogullari ME. (2005). The influence of various conditioner agents on the interdiffusion zone and microleakage of a glass ionomer cement with a high viscosity in primary teeth. *Oper Dent*, 30, 105–12.
- [40] Glasspoole EA, Erickson RL, Davidson CL. (2002). Effect of surface treatments on the bond strength of glass ionomers to enamel. *Dent Mater*, 18, 454–62. [doi: 10.1016/s0109-5641(01)00068-9. PMID: 12098574].
- [41] Castro A, Feigal RE. (2002). Microleakage of a new improved glass ionomer restorative material in primary and permanent teeth. *Pediatr Dent*, 24, 23–8.
- [42] Aboush YE, Jenkins CB. (1987). The effect of poly (acrylic acid) cleanser on the adhesion of a glass polyalkenoate cement to enamel and dentine. *J Dent*, 15, 147–52. [doi: 10.1016/0300-5712(87)90138-2. PMID: 3312324].
- [43] Okada K, Tosaki S, Hirota K, Hume WR. (2001). Surface hardness change of re-storative filling materials stored in saliva. *Dent Mater*, 17, 34-39. [doi: 10.1016/s0109-5641(00)00053-1. PMID: 11124411].
- [44] Papacchini F, Goracci C, Sadek FT, Monticelli F, Garcia-Godoy F, Ferrari M. (2005). Microtensile bond strength to ground enamel by glass-ionomers, resin-modified glass-ionomers and resin composites used as pit and fissure sealants. *J Dent*, 33, 459-467. [doi: 10.1016/j.jdent.2004.11.007. Epub 2004 Dec 20. PMID: 15935265].
- [45] Smales RJ, Gao W, Ho FT. (1997). In vitro evaluation of sealing pits and fissures with newer glass-ionomers developed for the ART technique. *J Clin Pediatr Dent*, 21, 321-323.
- [46] Van Duinen RNB, Davidson CL, de Gee AJ, Feilzer AJ. (2004). In situ transformation of glass-ionomer into an enamel-like material. *Am J Dent*, 17, 223-227.